

RPFT^{Q&As}

Registry Examination for Advanced Pulmonary Function Technologists

Pass Test Prep RPFT Exam with 100% Guarantee

Free Download Real Questions & Answers **PDF** and **VCE** file from:


<https://www.leads4pass.com/rpft.html>

100% Passing Guarantee
100% Money Back Assurance

Following Questions and Answers are all new published by Test Prep
Official Exam Center

- ⚙️ **Instant Download** After Purchase
- ⚙️ **100% Money Back** Guarantee
- ⚙️ **365 Days** Free Update
- ⚙️ **800,000+** Satisfied Customers

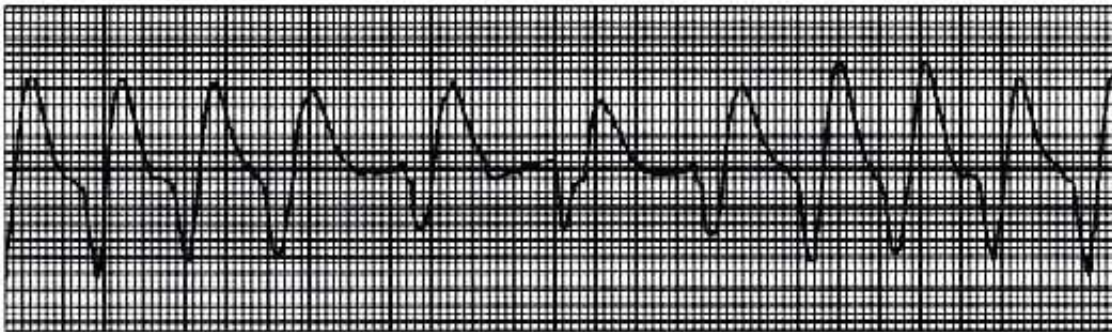

QUESTION 1

25 mm/sec




The ECG above is recorded during the recovery phase immediately following termination of an ergo meter exercise study. A pulmonary function technologist should

- A. Initiate chest compressions
- B. Have the patient lie down
- C. Check the electrode connections
- D. Continue the cool-down phase

Correct Answer: A

QUESTION 2

The following Levy-Jennings charts of control values are obtained: Which of the following is the correct sequence of actions for a pulmonary function technologist to take?

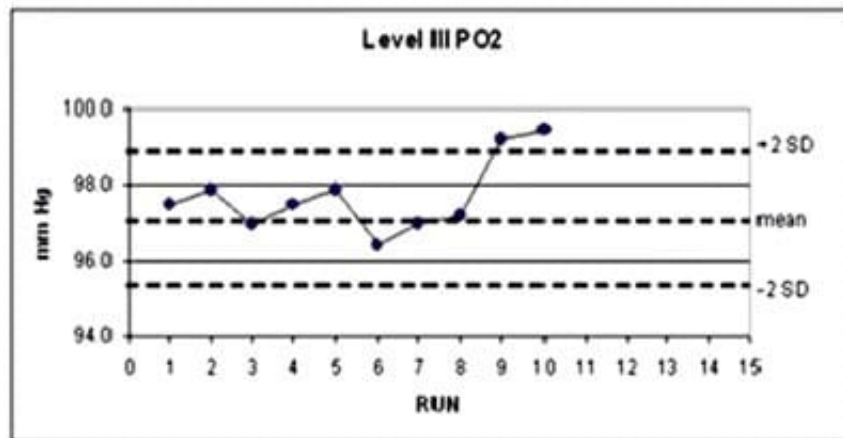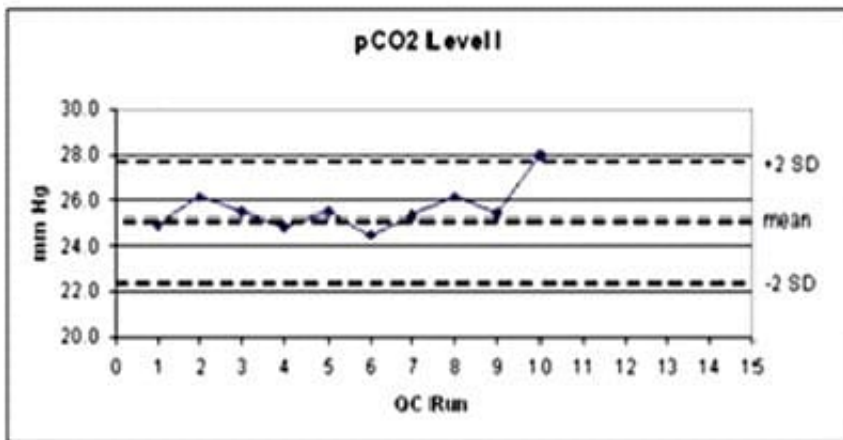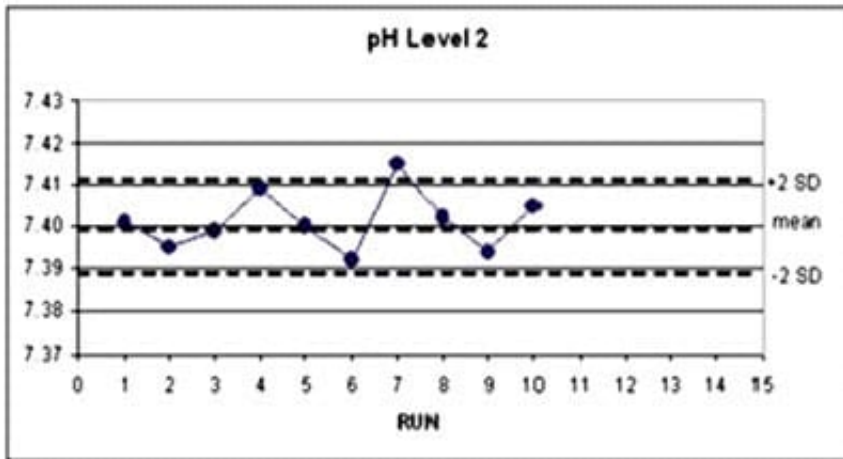

1.
Replace the oxygen electrode.
2.
Check the temperature of the measuring chamber.
3.
Run protein remover through the blood gas analyzer.
- 4.


Replace the CO₂ electrode.

- A. 3, then 1
- B. 1, then 4
- C. 2, then 3
- D. 4, then 2

Correct Answer: A

QUESTION 3

The following biologic control measurements are obtained:

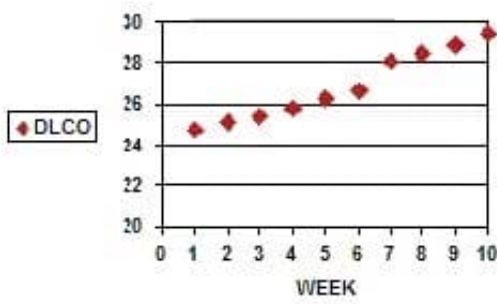


Which of the following patterns appears in this plot?

- A. Shift
- B. In control
- C. Drift
- D. Noise

Correct Answer: D

QUESTION 4

The following data were obtained from a bronchial challenge test:

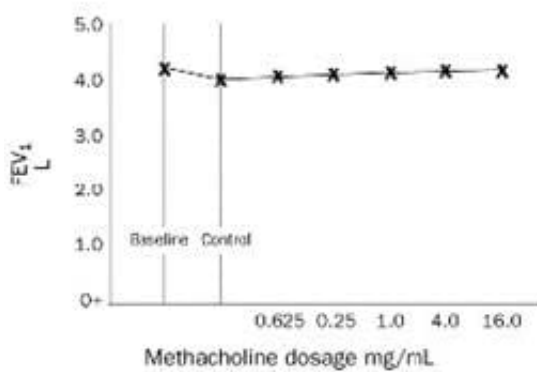

APC20 of 2 mg/mL was obtained the next day in another laboratory. Which of the following is the most likely explanation for these data?

- A. The two test results are within day-to-day variability.
- B. Incorrect doses of methacholine were administered.
- C. The spirometer accuracy drifted during the test.
- D. The patient's effort was inconsistent.

Correct Answer: C

QUESTION 5

The desiccant column on an infrared CO₂ analyzer is pink. The readings obtained from this analyzer would result in

- A. A decreased CO₂
- B. An increased CO₂
- C. An unstable reading
- D. No effect on CO₂

Correct Answer: B

[Latest RPFT Dumps](#)

[RPFT PDF Dumps](#)

[RPFT Exam Questions](#)